ÇİZGİ KUMPASI

ÖZELLİKLER

- ÖLÇEK 0,1 mm
- TEK PARÇA SÜRGÜLÜ
- PASLANMAZ ÇELİKTEN ÜRETİLMİŞTİR
- SERTLEŞTİRİLMİŞ ÖLÇÜM YÜZEYİ
- KALİBRASYON SERTİFİKASI

AS-322720

KOD	KAPASİTE	ÖLÇEK	HASSASİYET	ÇENE UZUNLUĞU
AS-322710	0-150 mm	0,1 mm	±0,2 mm	40 mm
AS-322720	0-200 mm	0,1 mm	±0,3 mm	40 mm
AS-322730	0-250 mm	0,1 mm	±0,3 mm	40 mm
AS-322740	0-300 mm	0,1 mm	±0,3 mm	40 mm

ASIMETO KALİBRASYON LABORATUARI

Tüm ASIMETO Hassas Ölçü Aletlerinin kalite ve kalibrasyon doğruluğu ASIMETO kalibrasyon laboratuarında hassas incelemelerle yapılmaktadır.

İncelemeler sırasında tüm hassas ölçü aletlerinin ASIMETO tarafından oluşturulan dizayn ve Dünya çapında standartlarla belirlenen toleranslara uygunluğu %100 olarak kontrol edilir.

Yalnızca Dünya'nın önde gelen firmaları tarafından üretilen son teknoloji kalibrasyon ekipmanları kullanılarak ASIMETO Hassas Ölçü Aletlerinin ölçüm hassasiyeti garanti altına alınır.

ASIMETO Kalibrasyon Laboratuarındaki kalibrasyon ekipmanları hedef marketin ihtiyacına göre DIN, ASME, JJG gibi Uluslararası normların tamamına uyum gösterecek yazılımlarla donatılmıştır.

Tüm bu sayılanlara ASIMETO kalibrasyon laboratuarında çalışanların uzmanlık, özveri ve çalışkanlıkları da eklendiğinde ihtiyacınızı karşılayacak hassasiyetteki ölçü aletine ödediğiniz her kuruşun karşılığını tamı tamına alacak şekilde sahip olduğunuza emin olabilirsiniz.

ASIMETO
Calibration Lab

ilac-MRA CNAS
China National Accreditation Service for Conformity Assessment
LABORATORY ACCREDITATION CERTIFICATE
(Registration No. CNAS L6296)
Calibration Laboratory of Guangzhou Asimeto Measuring Instrument Co., Ltd.
Room 402, Building B, Fukang West Street, Yushu Industrial Zone, Science Area, Luogang District, Guangzhou, Guangdong, China
is accredited in accordance with ISO/IEC 17025:2005 General Requirements for the Competence of Testing and Calibration Laboratories(CNAS-CL01 Accreditation Criteria for the Competence of Testing and Calibration Laboratories) for the competence to undertake the service described in the schedule attached to this certificate.
The scope of accreditation is detailed in the attached schedule bearing the same registration number as above. The schedule form an integral part of this certificate.
Date of Issue: 2016-08-01
Date of Expiry: 2022-07-21
Date of Initial Accreditation: 2013-07-22
Signed on behalf of China National Accreditation Service for Conformity Assessment

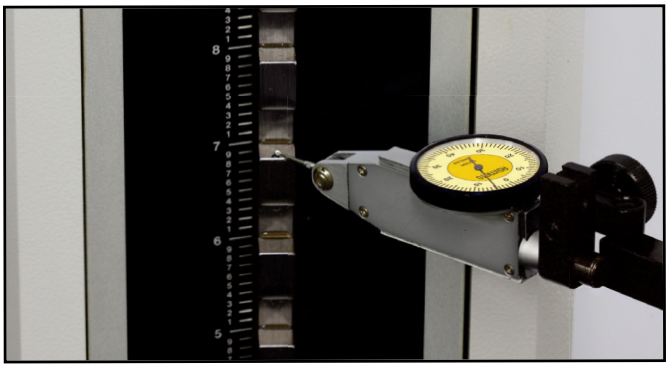

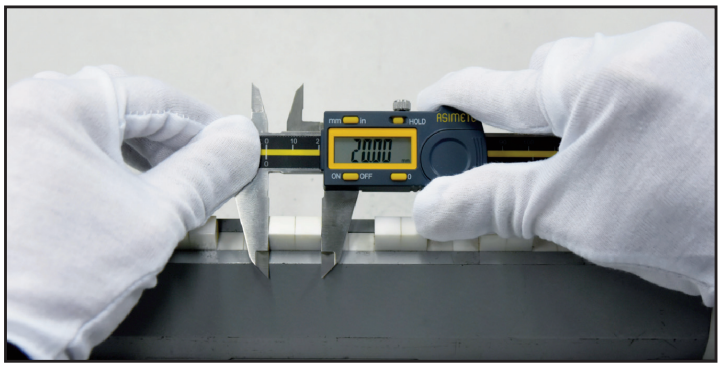

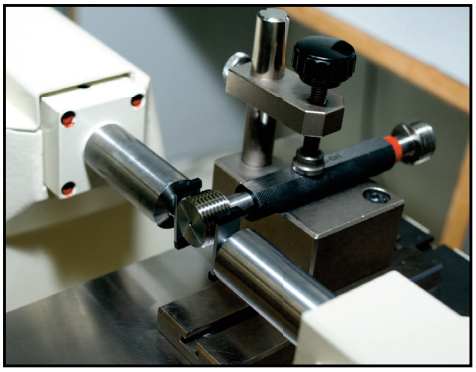

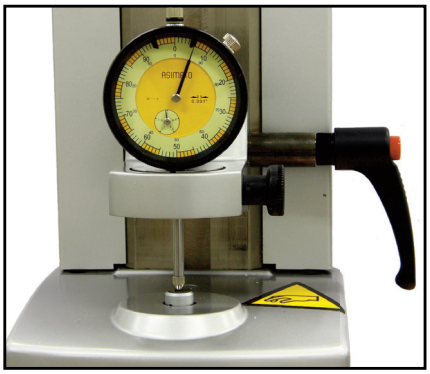

2 Ürün Açıklaması

1 Ölçüm Noktası & Sonuç

3 Eğilim

4 Takip No.

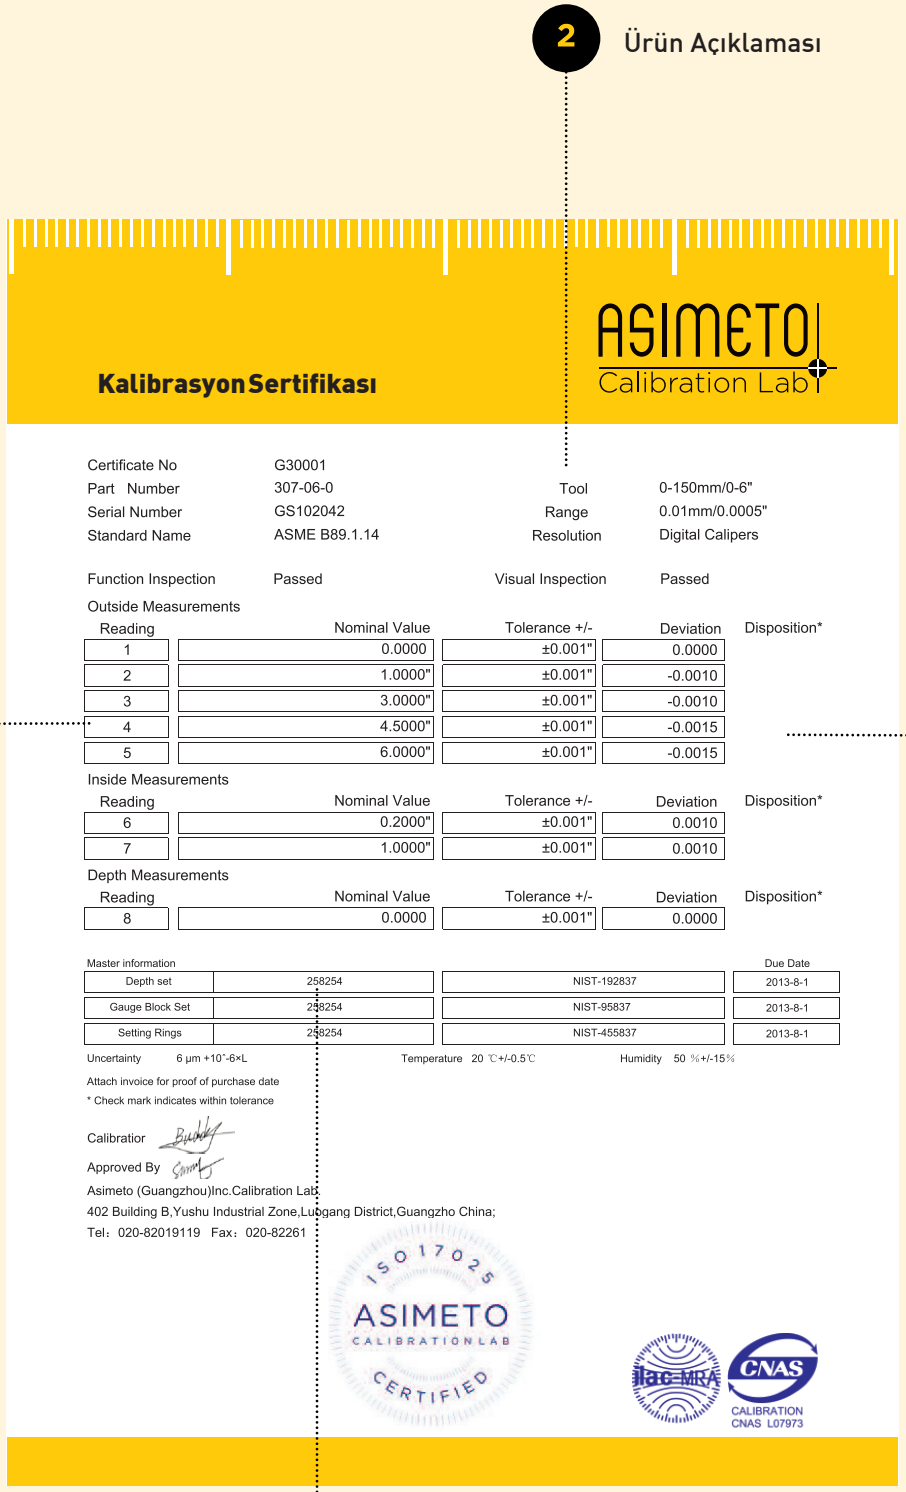

Kalibrasyon Sertifikası

ASIMETO Calibration Lab

Certificate No	G30001		
Part Number	307-06-0	Tool	0-150mm/0-6"
Serial Number	GS102042	Range	0.01mm/0.0005"
Standard Name	ASME B89.1.14	Resolution	Digital Calipers
Function Inspection	Passed	Visual Inspection	Passed

Outside Measurements

Reading	Nominal Value	Tolerance +/-	Deviation	Disposition*
1	0.0000	±0.001"	0.0000	
2	1.0000"	±0.001"	-0.0010	
3	3.0000"	±0.001"	-0.0010	
4	4.5000"	±0.001"	-0.0015	
5	6.0000"	±0.001"	-0.0015	

Inside Measurements

Reading	Nominal Value	Tolerance +/-	Deviation	Disposition*
6	0.2000"	±0.001"	0.0010	
7	1.0000"	±0.001"	0.0010	

Depth Measurements

Reading	Nominal Value	Tolerance +/-	Deviation	Disposition*
8	0.0000	±0.001"	0.0000	

Master information			Due Date
Depth set	258254	NIST-192837	2013-8-1
Gauge Block Set	258254	NIST-95837	2013-8-1
Setting Rings	258254	NIST-455837	2013-8-1

Uncertainty 6 μm +10^-6×L Temperature 20 ℃+/-0.5℃ Humidity 50 %+/-15%

Attach invoice for proof of purchase date

* Check mark indicates within tolerance

Calibratior

Approved By

Asimeto (Guangzhou)Inc.Calibration Lab

402 Building B,Yushu Industrial Zone,Luogang District,Guangzho China;

Tel：020-82019119 Fax：020-82261

ISO 17025 ASIMETO CALIBRATION LAB CERTIFIED

ilac-MRA CNAS CALIBRATION CNAS L07973

Bilgi Çıkışlı Ölçü Aletleri

ABS Dijital Kumpas

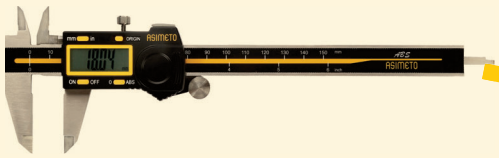

Derinlik Kumpası

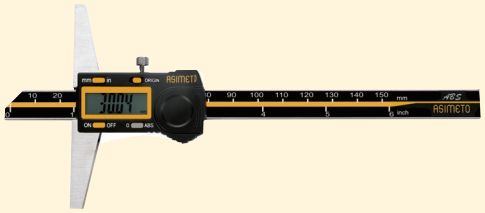

Dijital Mikrometre

Dijital Komparatör Saati

Sanal klavye verileri toplar ve doğrudan standart Microsoft yazılımlarına iletir. (Excel, Access)

Ölçüm Raporu

	A1	A2	A3
1	10.02	15.53	20.44
2	10.04	15.53	20.46
3	10.01	15.52	20.44
4	10.01	15.53	20.45
5	10.02	15.54	20.46
Average	10.02	15.53	20.45

BİLGİ ÇIKIŞ KABLOLARI 900 SERİSİ

	UYGUN OLDUĞU ÜRÜN	GİRİŞ TİPİ	FORMAT	UYGUN OLDUĞU ÜRÜN	KOD NO.
	ABS Dijital Kumpas Dijital Mikrometre Ağır İş Dijital Kumpas	USB	Dot Data Format	307-XX-2 ; 307-XX-3 105-XX-4 ; 105-XX-5 315-XX-6 ; 315-XX-8	**900-05-4**
			Comma Data Format		**900-05-5**
	IP65 Dijital Komparatör Saati	USB	Dot Data Format	407-XX-2 ; 407-XX-3 407-XX-4 ; 407-XX-5	**900-07-0**
			Comma Data Format		**900-07-1**
	Dijital Komparatör Saati	USB	Dot Data Format	405-95-X ; 405-01-X 405-02-X ; 405-04-X	**900-20-0**
	Dijital Mikrometre	USB	Dot Data Format	Özel Dijital Mikrometre	**900-10-0**
	Dijital Mikrometre	USB	Dot Data Format	Özel Dijital Mikrometre	**900-10-2**
	Wireless Tip İçin Ayak Kontrol Butonu				**900-90-1**

KABLOSUZ BİLGİ ÇIKIŞ TİPLERİ 901 SERİSİ

	KULLANILDIĞI ÜRÜN TİPİ	FONKSİYON	FREKANS	KOD NO.
	IP65 Dijital Komparatör Saati	Transmitter	2.4G	**901-00-2**
	IP65 Dijital Komparatör Saati ABS Dijital Kumpas Dijital Mikrometre Ağır İş Dijital Kumpas	Receiver	2.4G	**901-00-3**
	ABS Dijital Kumpas Dijital Mikrometre Ağır İş Dijital Kumpas	Transmitter	2.4G	**901-00-4**
	ABS Dijital Kumpas Dijital Mikrometre Ağır İş Dijital Kumpas	Transmitter with Footswitch Interface	2.4G	**901-00-6**
	IP65 Dijital Komparatör Saati	Transmitter with Footswitch Interface	2.4G	**901-00-7**